

PREPARATION OF SECONDARY pH OF PHTHALATE BUFFER SOLUTION USING DIFFERENTIAL POTENTIOMETRIC CELL: METHOD VALIDATION AND APPLICATION

*Ayu Hindayani¹, Oman Zuas^{1, *}, Sujarwo², Fransiska S. H. Krismastuti², Nuryatini¹*

<https://doi.org/10.23939/chcht13.03.377>

Abstract. A secondary pH of phthalate buffer was prepared by differential potentiometry method using a Baucke cell which is separated by sintered glass disk in the middle of cell – so called two-half cells. The method has been validated at 298 K with the purpose to evaluate its suitability for meeting the application requirement. The method validation parameters include accuracy (bias), precision (repeatability), and estimation of measurement uncertainty. It was found that both accuracy and precision of the method were good, which is indicated by their very low standard deviation (SD). The measurement uncertainty value of the method was estimated. Application of the validated analytical method for the measurement of phthalate buffer in an international comparative test (APMP.QM-K91) showed that the result was close to the APMP.QM-K91's Key Comparison Reference Value.

Keywords: differential potentiometric cell, pH, phthalate buffer, method validation, international key comparison.

1. Introduction

Scientifically, pH is defined as a value of $-\log a_H$, involving a single ion quantity and activity of hydrogen ion [1]. Practically, the pH is used to specify acidity or basicity properties of any substance that are mainly in the form of their aqueous solution. Determination of pH is one of the most common and frequent quantitative measurement in the field of chemical analyzes [2]. The

common application of the pH measurement is to control industrial processes with the purposes to preserve product quality, reduce the corrosion rate in plant equipment, and protect the aqueous environment by helping wastewater discharge process to meet regulatory limits [3].

Measurement of pH is a process applying the physico-chemical principle and it can be performed by using various methods such as colorimetry and potentiometry. To date, potentiometry is widely used due to its simplicity and accuracy in comparison to other methods [4]. Potentiometric method is measuring the potential difference between two electrodes that are simultaneously immersed in the solution to be examined [5], by which those glass electrodes must be regularly calibrated before use by using pH buffer standard solution.

A reliable data of a pH measurement process having a traceability property to the International System of Units (SI) is extremely required [2]. For pH measurement, the traceability chain can be established by linking the pH data resulted from a measurement to the pH value of a primary pH buffer standard solution [6]. This buffer standard is obtained from the primary method [2]. It is widely known that the primary pH buffer standard solution for the calibration purpose is characterized by its long-term stability, high purity and good reproducibility [6]. However, the use of primary pH buffer standard solution by common testing and calibration laboratories is costly; thus secondary pH buffer standard solution is an alternative which is widely used by the laboratories to keep the traceability of their pH measured data [2].

So far, the pH value of secondary pH standard buffer solution is commonly determined by secondary method using differential potentiometric cell or called as Baucke cell. This method was firstly introduced in 1994 by F. Baucke, whose name was then used for naming the cell [2]. Schematic design of Baucke cell is presented in Fig. 1 [6].

¹ Metrology in Chemistry Laboratory, Centre for Research and Human Resource Development, National Standardization Agency of Indonesia (BSN), Kawasan PUSPIPTEK Build. 420, Serpong15314, Tangerang Selatan-Banten, Indonesia

² Research Centre for Chemistry-Indonesian Institute of Sciences (RCChem-LIPI)

Kawasan PUSPIPTEK Build. 452, Serpong15314, Tangerang Selatan-Banten, Indonesia

* oman@bsn.go.id; zuas.oman@gmail.com

© Hindayani A., Zuas O., Sujarwo, Krismastuti F., Nuryatini, 2019

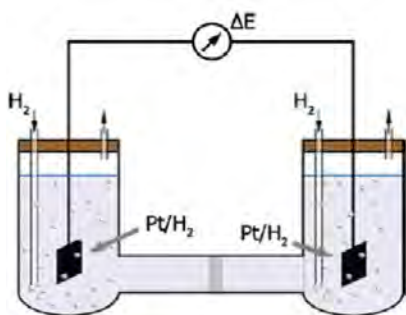


Fig. 1. Schematic diagram of Baucke cell [6]

Baucke cell is U-shaped cell separated by a sintered glass disk in the middle of the cells, called as two-half cells. One cell contains the primary buffer solution (as a standard solution) and platinum/hydrogen (Pt/H₂) electrode. Another cell contains secondary buffer solution (as a sample solution) and Pt/H₂ electrode. These two buffer solutions must have the same nominal composition. Similarly, two Pt/H₂ electrodes must have as similar characteristic as possible. Since the hydrogen in the half cells is about the same, liquid junction potential (LJP, developed in the junction between the two half cells) can be neglected [2]. The pH of secondary buffer can be calculated by Eq. (1) [2]:

$$\text{pH}_s = \text{pH}_p - \frac{\Delta E_{\text{cell}} F}{RT \ln 10} \quad (1)$$

where pH_p is pH value from primary buffer standard solution; ΔE_{cell} is potential difference between two Pt/H₂ electrodes after stabilization (V); F is Faraday constant (96,485 C·mol⁻¹), R is the universal gas constant (8.314 J·K⁻¹·mol⁻¹); T is solution temperature (K) [2].

In Indonesia, most of industrial and testing laboratories used imported and traceable buffer standard solutions in their pH measurement activities [7]. The use of traceable secondary pH buffer standard solutions is extremely important to keep the traceability of the measurement to the SI unit. However, an imported buffer standard solution is economically disadvantageous due to being costly and the import process is also time consuming. Therefore, providing the industries and testing laboratories with secondary buffer standard solution to meet the local need is essential.

In pH measurement, the phthalate buffer is one of the most commonly used in comparison to other buffer standard solutions because it is readily commercial available, relatively stable and pH value is markedly non-sensitive to a temperature change [8]. In addition, the phthalate buffer standard solution can be easily prepared from readily available certified material.

In this study, a phthalate buffer solution as a secondary pH buffer standard solution was developed by

LIPI. The secondary pH buffer standard solution was prepared by using gravimetric method and the pH values were determined by the differential potentiometry method using a Standard Reference Material[®] potassium hydrogen phthalate (SRM[®] 185i) as the traceable reference standard. It is important to notice that methods for the preparation and pH measurement must be validated before determining the pH value and producing the phthalate buffer solution in a large scale. The purpose of the method validation is not only to meet its suitability requirement for application but also to evaluate the method's performance [9], by which the results are presented and discussed in this paper.

2. Experimental

2.1. Materials

All chemicals were of analytical grade, otherwise stated, and used as received without any further purification. Hydrogen (H₂) gas (99.9 % purity) was purchased from SII Gas Indonesia. Chloride acid (37 % purity), nitric acid (65 % purity), lead (II) acetate (99.5 % purity), Certipure[®] Certified Reference Material (CRM) potassium hydrogen phthalate (1019650025) were purchased from Merck, Germany. Palladium (II) chloride (anhydrous, Pd basis 60 %) was purchased from Sigma-Aldrich, USA. The SRM[®] 185i was purchased from National Institute of Standards and Technology (NIST), USA. Demineralized water (0.05 μs/cm) was produced from a Thermo Scientific Barnsted Smart2 pure water purification system and used in all experiments.

2.2. Equipment

For the investigations we used: analytical balance with accuracy of 1 mg (PR5003 Dual Range, Mettler Toledo Switzerland), oven (Heraeus Instruments, Germany) and a direct current (DC) power supply 0.01 A (Ad-8723D, China), a digital multimeter 0.01 mV (34461A, Agilent Technologies Sdn Bhd, Malaysia), waterbath 0.1 K (Thomas T-N22D, Japan), chiller (Thomas TRL-117NF, Japan), hot plate and magnetic stirrer (Cimarec 2, Barnstead Thermolyne Corp. USA), fume hood (LFH-2120V, Daihan Labtech Korea), digital thermometer (MKT50, Anton Paar GmbH, Germany), Baucke Cell, Pt electrode, and chamber (Japan), stopwatch, and clean glasswares.

2.3. Procedure

2.3.1. Preparation of buffer solution

Standard buffer solution was made from phthalate buffer solution (0.05 molal) SRM[®] 185i by adopting a

procedure from [10]. In a typical experiment, the SRM[®]NIST 185i was firstly dried at 383.15 K for 2 h followed by storing in a desiccator until use, aiming to remove the water content because the SRM[®] 185i is stable only in a dry environment. After that, 9.8 g of SRM 185i was transferred into a clean and dry beaker glass (1 l). Demineralized water was then added into the beaker glass until the mass reach 959.293 g. The solution was shaken thoroughly until the solid was totally dissolved. This gravimetric preparation could eliminate the need to weigh exactly predetermined mass of solid samples.

Another buffer solution (0.05 molal), as a sample, was made from Certipure[®] CRM potassium hydrogen phthalate in accordance with the procedure described in [11]. The CRM was dried by placing in an oven at 383.15 K for 2 h in order to remove the water content. After that, 10.21 g of CRM was dissolved in 800 ml of water and made up to 1 l. The solution was shaken thoroughly until the solid was totally dissolved.

2.3.2. Preparation of Pt electrode

The use of clean Pt electrodes in pH measurements by differential potentiometric cell is considered very important. In this study, the Pt electrodes were cleaned using hot aqua regia in order to achieve a sufficiently small of potential bias [12] and to remove any impurities from the electrode surface, by which the possible interference during the measurement can be diminished [13]. After that, a palladinizing process for the Pt electrode to minimize reduction of phthalate was carried out by coating method using palladium black solution [8]. Typically, palladium black solution was a solution mixture consisting of palladium chloride, lead acetate and chloride acid, where the Pt electrodes were coated by electrolytic method [12]. The presence of the palladium black on the electrode surface may increase the effectiveness of a hydrogen electrode [14]. Preliminary results showed that a slightly coated electrode surface was found to be more stable than thick coated one [8]. To determine the best surface coating of the electrodes, the effect of palladinizing parameters such as current and time were studied. The variation of the current and time was ranging within 0.3–0.5 A and 2–5 min, respectively.

2.3.3. pH Measurements

The pH of phthalate buffer 0.05 molal (both standard and sample) were measured by using differential potentiometric cell. The potential difference between SRM[®]185i as a standard and Certipure[®] CRM potassium hydrogen phthalate as a sample was assigned as ΔE_{cell} . Both buffer solutions were placed in the Baucke cell, followed by inserting the palladinized Pt electrodes into each cell. After that, the Baucke cell was immersed into

the waterbath (298 K). The hydrogen gas was then fed into each cell with the flow rate of 500 ml/h [12]. It should be noticed that the hydrogen gas was firstly pre-humidified before entering the Baucke cell by passing through the hydrogen into two chambers containing phthalate buffer solution [2]. The palladinized Pt electrodes were then connected to digital multimeter and the ΔE_{cell} value was recorded after stabilization. A schematic diagram of the differential potentiometric cell system used in this study is shown in Fig. 2. In this study, one hour was required to stabilize the potential and the measurement was then conducted every 10 min. Finally, the mean value of ΔE_{cell} was used for calculating the pH values by using Eq. (1).

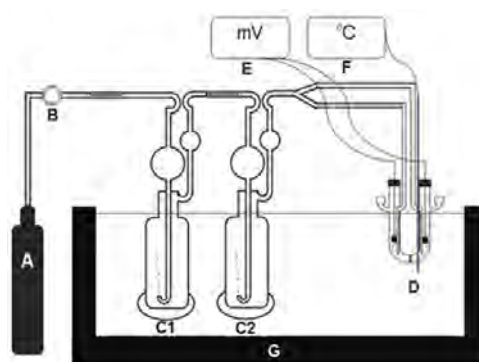


Fig. 2. Schematic diagram of differential potentiometric cell system: hydrogen gas (A), gas controller (B), chambers containing phthalate buffer (C1 and C2), Baucke cell and Pt electrodes (D), digital multimeter (E), digital thermometer (F) and water bath (G)

2.3.4. Validation method

Validation of an analytical method is a process of defining an analytical requirement and confirming that the method under consideration has capabilities and is consistent with its application requirements [9]. In this study, differential potentiometric cell was used for the preparation of secondary reference material for pH measurement; thus, validation of the method is extremely required to meet its application purposes. In general, validations of the method are conducted to evaluate the performance characteristics of the method in term of its selectivity, limit of detection (LOD) and limit quantification (LOQ), working range, analytical sensitivity, accuracy (bias), precision (repeatability), robustness, and estimation of measurement uncertainty [9]. However, in analytical pH measurement, the validation method is only limited to such parameters as accuracy (bias), precision (repeatability) and measurement of the uncertainty.

Accuracy is referred to how close the mean of measurement result (produced by method) is to the

reference value. This assessment is commonly quantitatively expressed as bias [9]. Determination of bias (b) relies on the different between the mean of measurement results (\bar{X}) and the reference value stated in CRM's certificate (X_{CRM}). The value of b is determined by using Eq. (2) [9].

$$b = |\bar{X} - X_{CRM}| \quad (2)$$

In this study, the mean from 10 times of measurements was used. The method is categorized as not to be bias, when the value falls within the range of measurement precision value ($\pm 2S$) (Eq. (3)) with calculation of S (Eq. (4)) at 95% confidence level [15].

$$-2S < b < +2S \quad (3)$$

$$S = \sqrt{U_{CRM}^2 + \frac{S_w^2}{n}} \quad (4)$$

where U_{CRM} is standard uncertainty from certificate; S_w is standard deviation, and n is a number of measurements.

Precision (also called as repeatability) is a measure of how close the measurement results are one to another [9]. Precision is usually expressed by a standard deviation obtained from several measurement replications. In the pH measurement using differential potentiometric cell, a good repeatability is achieved when the value of standard deviation is equal or less than $6.0 \cdot 10^{-5}$ V. This criterion is based on our experiences in the measurement using differential potentiometric cell to decrease the measurement uncertainty.

Moreover, for estimating the uncertainty of the measurement, identification of the uncertainty sources which contribute to the measurement uncertainty value is the initial step. After that, estimation of the uncertainty from each individual source was conducted followed by combining such individual uncertainties to give an overall estimation of measurement uncertainty [16].

3. Results and Discussion

In the BSN, the electrochemistry laboratory is a part of metrology in chemistry group which has responsibility for the development of reference material in electrochemistry field such as buffer. The developed buffer reference materials are used to keep the traceability of pH measurement (at national level) to SI. It might be an acceptable idea that every method must be validated before coming into use for a routine measurement. In this study, the measurement of the phthalate buffer was determined by secondary method using differential potentiometric cell and the method was validated in term of the measurement accuracy (bias), precision (repeatability), and its measurement uncertainty estimation.

3.1. Palladinizing Pt Electrodes

Optimization of palladinizing Pt electrode is an important step and it has to be conducted to increase the work efficiency of the Pt electrode, because in homogeneities such as tiny spots on the electrode surface may affect the measurement results. Therefore, any surface dirt must be removed by cleaning procedure [12]. Besides, in the differential potentiometry, the surface condition of two Pt electrodes must be as similar as possible [2].

Fig. 3 shows the ΔE_{cell} dependency on the electrical current used in the palladinizing Pt electrode. It can be seen from Fig. 3 that the obtained ΔE_{cell} value significantly decreases when the electrical current increases up to 0.4 A and then increases. This phenomenon can be described as follows: at a low current (below 0.4 A) in palladinizing, only a small number of metal was deposited on the surface of Pt electrode and that was a non-optimum condition to minimize the reduction process of phthalates, leading to a very large ΔE_{cell} value. In contrast, at a high current (above 0.4 A), the ΔE_{cell} value is significantly increased. These high ΔE_{cell} values might be due to the high current used in the palladinizing resulting in inhomogeneity of deposited metal on the electrode surface [17]. Consequently, two Pt electrodes were unidentical and those electrodes did not meet the requirement of the electrodes used in potential differential potentiometric cell. Moreover, when palladinizing at the current of 0.4 A, the ΔE_{cell} was found to be the smallest value, indicating that two half cells were similar, having homogenous deposition of metal on the electrode surface. Based on this finding, a value of 0.4 A was used as the optimal current in palladinizing the Pt electrodes.

Fig. 4 displays the effect of time variation on the ΔE_{cell} value. As it can be seen from Fig. 4, ΔE_{cell} decreases in 2–4 min and then increases in 5 min. For 2 min, the ΔE_{cell} was found to have a relatively high value. It was assumed that due to the short time of palladinizing process a very small amount of metal is deposited on the electrode surface (data are not shown here). Thus, the reduction of phthalates cannot be minimized. On the contrary, longer palladinizing time may decrease the ΔE_{cell} value and the lowest value of ΔE_{cell} is achieved in 4 min, indicating that the metal deposited on the electrode surface was in a homogenous and optimum condition. Consequently, the smallest ΔE_{cell} value confirms that the optimum palladinizing time is 4 min.

So, it can be concluded that the optimum electrical current and reaction time were 0.4 A and 4 min, respectively. The Pt electrode obtained under this optimum condition was then used for the measurements in the validation of the analytical method.

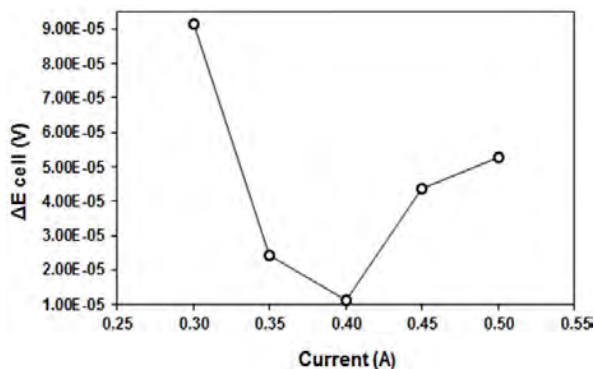


Fig.3. The dependence of ΔE_{cell} on the electrical current in Pt electrodes palladinizing

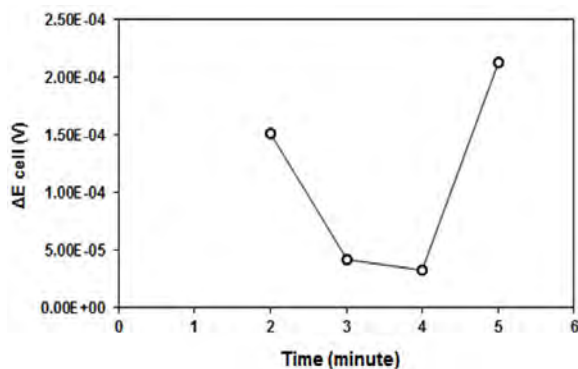


Fig. 4. Optimization of time in Pt electrodes palladinizing

3.2. Validation Method

In this study, the validation of the measurement method was conducted in terms of accuracy (bias), precision (repeatability) and measurement uncertainty estimation. For the accuracy, the evaluation was taken by estimating the bias of the mean true value from 10 measurement replications. The results of the method accuracy are presented in Table 1. It can be seen from Table 1 that the mean of pH value of the CRM was found to be 4.0052, while the certificate value of the secondary phthalate buffer was 4.0070; thus the bias of the method was 0.0018. This bias value is relatively small and lies in the range of the precision value $\pm 2\sigma$ (with 95% confidence level), implying that the analytical method is accurate [15].

Table 1

Accuracy data of the analytical method

| Measurements | pH at 298 K |
|---|-----------------------------|
| 1 | 4.0045 |
| 2 | 4.0051 |
| 3 | 4.0050 |
| 4 | 4.0056 |
| 5 | 4.0057 |
| 6 | 4.0057 |
| 7 | 4.0053 |
| 8 | 4.0056 |
| 9 | 4.0050 |
| 10 | 4.0049 |
| Mean (\bar{X}) | 4.0052 |
| Standard deviation (S_w) | 0.0004 |
| U_{CRM} | 0.0015 |
| X_{CRM} | 4.0070 |
| $b = \bar{X} - X_{CRM} $ (Eq. 2) | 0.0018 |
| $\sigma = \sqrt{U_{CRM}^2 + \frac{S_w^2}{n}}$ (Eq. 4) | 0.0015 |
| Criteria $-2S \ll$ (Eq. 3) | $-0.0030 < 0.0018 < 0.0030$ |
| Status | OK |

Precision (repeatability) is a measure of how close the measurement results are to each other [9]. The precision is usually expressed by standard deviation from several measurement replications. In this study, repeatability was carried out by measure of the sample in 10 replications and the results are listed in Table 2. From the Table 2, it was found that the standard deviation for the measurement is $3.0 \cdot 10^{-5}$ which is lower than acceptance criteria value ($6.0 \cdot 10^{-5}$ V) of our experience in measurement using differential potentiometric cell. Hence, it can be concluded that the analytical method used in this study is precise (repeatability). Moreover, for the measurement uncertainty estimation, all possible sources of the uncertainty contributor were identified and schematically displayed using Ishikawa diagram as shown in Fig. 5 [2].

Table 2

Precision/repeatability data of the analytical method

| Measurements | ΔE_{cell} at 298 K, V |
|------------------------------|--|
| 1 | 0.00009 |
| 2 | 0.00001 |
| 3 | 0.00005 |
| 4 | 0.00004 |
| 5 | 0.00002 |
| 6 | 0.00005 |
| 7 | 0.00008 |
| 8 | 0.00008 |
| 9 | 0.00001 |
| 10 | 0.00008 |
| Mean (\bar{X}) | 0.00005 |
| Standard deviation (S_w) | $3.0 \cdot 10^{-5}$ |
| Criteria | equal or less than $6.0 \cdot 10^{-5}$ |
| Status | OK |

Table 3 shows the measurement uncertainty estimation for secondary pH measurement. From Table 3, it can be seen that the expanded uncertainty for the secondary pH measurement using differential potentiometric cell is within the acceptance criteria.

metric cell at 298 K is 0.001 (95 % confidence level), which is lower than the IUPAC recommended value (0.004 at 95 % confidence level) [1]. Extremely small uncertainty of the primary buffer used might be the reason for small uncertainty obtained in this study, indicating that uncertainty of the primary buffer is very important [2].

3.3. Application

Validation method of the secondary pH measurement using differential potentiometric cell is to check

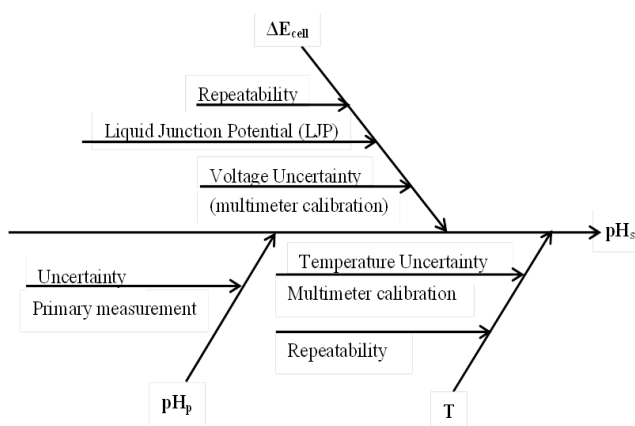


Fig. 5. Ishikawa diagram [2]

the suitability of the differential potentiometry method with the application required and evaluate the method's performance. In this regard, participation in an international key comparison (APMP.QM-K91) was conducted. In short, the comparison results indicated that differential potentiometric cell can be used in the pH measurements of phthalate buffer at 298 K. The measured value (4.006) is close to the APMP.QM-K91's key comparison reference value (KCRV), that is 4.00765. The results are graphically displayed in Fig. 6 [18].

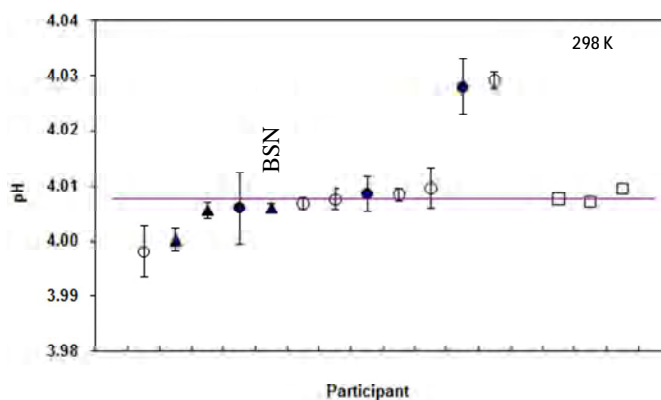


Fig. 6. Results of pH measurements of phthalate buffer at 298 K compared with APMP.QM-K91 [18]

Table 3

Data for uncertainty estimation of secondary pH measurement using differential potentiometric cell at 298 K

| Sources | Standard uncertainty (u_i) | Unit | Sensitivity coefficient (c_i) | Unit | $u_i \cdot c_i$ |
|-------------------|--------------------------------|------|-----------------------------------|---------------------------------------|-----------------------|
| Primary buffer | 0.0004 | – | 1 | – | 0.0004 |
| ΔE_{cell} | | | | | |
| $E_{cal.}$ | $5.50 \cdot 10^{-7}$ | V | -16.91 | V^{-1} | $-9.30 \cdot 10^{-6}$ |
| $E_{res.}$ | $5.77 \cdot 10^{-7}$ | V | -16.91 | V^{-1} | $-9.76 \cdot 10^{-6}$ |
| $E_{stab.}$ | $2.00 \cdot 10^{-5}$ | V | -16.91 | V^{-1} | $-3.38 \cdot 10^{-4}$ |
| Repeatability | $3.23 \cdot 10^{-6}$ | V | -16.91 | V^{-1} | $-5.46 \cdot 10^{-5}$ |
| LJP | $3.53 \cdot 10^{-6}$ | V | -16.91 | V^{-1} | $-5.96 \cdot 10^{-5}$ |
| Temperature | | | | | |
| $T_{cal.}$ | 0.02 | K | $2.0 \cdot 10^{-6}$ | K^{-1} | $3.0 \cdot 10^{-8}$ |
| $T_{res.}$ | 0.06 | K | $2.0 \cdot 10^{-6}$ | K^{-1} | $1.15 \cdot 10^{-7}$ |
| Stability | 0.06 | K | $2.0 \cdot 10^{-6}$ | K^{-1} | $1.20 \cdot 10^{-7}$ |
| Homogeneity | 0.04 | K | $2.0 \cdot 10^{-6}$ | K^{-1} | $8.0 \cdot 10^{-8}$ |
| | | | | Combined uncertainty (u_c) | 0.0005 |
| | | | | Expanded uncertainty (U), $k = 2$ | 0.001 |

4. Conclusions

The result of validation shows that the differential potentiometry method is appropriate for the pH measurement of phthalate buffer at 298 K, with the value of the bias and precision found to be 0.0018, and $3.0 \cdot 10^{-5}$, respectively, having an estimated uncertainty value of 0.001 ($k = 2$). The validated method of pH has been tested by participating in the international comparison (APMP.QM-K91) and the result was excellent, confirming that the method is valid.

Acknowledgments

The author would like to thank Mrs. Eli Susilawati for the help during laboratory experiments and data collection. The LIPI support of the study through the project "Strengthening chemical metrology competency and infrastructure" is highly acknowledged.

References

- [1] Buck R., Rondinini S. *et al.*: Pure Appl. Chem. 2002, **74**, 2169. <https://doi.org/10.1351/pac200274112169>
- [2] Gonzaga F., Dias J., Jehnert D. *et al.*: Electroanal., 2013, **25**, 1955. <https://doi.org/10.1002/elan.201300135>
- [3] Laongsri B., Boonyakong C., Tangpaisarnkul N., Cherdchu C.: Accred. Qual. Assur., 2017, **12**, 194. <https://doi.org/10.1007/s00769-006-0210-0>
- [4] Wu Y., Koch W., Marinenko G.: J. Res. Nat. Bur. Stand., 1984, **89**, 395.
- [5] European Pharmacopoeia, 4th edn. Council of Europe, Strasbourg 2002.
- [6] Spitzer P., Pratt K.: J. Solid State Electrochem., 2011, **15**, 69. <https://doi.org/10.1007/s10008-010-1106-9>
- [7] Nuryatini, Sjarwo, Hindayani A.: J. Standardisasi, 2015, **18**, 35.
- [8] Hetzer H., Durst R.: J. Res. Nat. Bur. Stand., 1977, **81A**, 21.
- [9] Magnusson B., Örnemark U. (Eds.): Eurachem Guide: The Fitness for Purpose of Analytical Methods – A Laboratory Guide to Method Validation and Related Topics, 2nd edn., 2014. www.eurachem.org.
- [10] Gonzalez C., Watters Jr. R.: Certificate of Analysis SRM[®]NIST 185i Potassium Hydrogen Phthalate pH Standard, Department of Commerce United States of America 2013.
- [11] Yildirim A.: Certificate of Analysis Certipure[®] Certified Reference Material Potassium Hydrogen Phthalate, MERCK, Germany 2015.
- [12] Baucke F.: J. Electroanal. Chem., 1994, **368**, 67. [https://doi.org/10.1016/0022-0728\(93\)03024-J](https://doi.org/10.1016/0022-0728(93)03024-J)
- [13] Mustopo Y.: Effect of Time on Thickness and Adhesivity Layer in Electroplating Process of Chrome Decorative without Basic Layer with Copper Basic Layer and Copper-Nickel., Department of Mechanical Engineering, Technical Faculty of UNS, Solo, Indonesia 2011.
- [14] Hamer W., Acree S.: J. Res. Nat. Bur. Stand., 1944, **33**, 87.
- [15] Budiman H.: Warta Kimia Analitik., 2014, **20**, 18.
- [16] Bell S.: Measurement Good Practice Guide (Issue 2), National Physical Laboratory, United Kingdom 2001.
- [17] Subangga B., Sutikno E., Ariseno A.: Effect of Anode Variation and time of Electroplating on Wear Rate of Grinding Ball., Department of Mechanical Engineering University of Brawijaya Malang.
- [18] Hioki A., Asakai T., Maksimov I. *et al.*: Metrologia, 2017, **54**, 08002. <https://doi.org/10.1088/0026-1394/54/1A/08002>

Received: March 13, 2018 / Revised: April 03, 2018 / Accepted: August 30, 2018

ПРИГОТУВАННЯ ВТОРИННОГО рН-СТАНДАРТУ ДЛЯ ФТАЛАТНОГО БУФЕРНОГО РОЗЧИНУ З ВИКОРИСТАННЯМ ДИФЕРЕНЦІАЛЬНОЇ ПОТЕНЦІОМЕТРИЧНОЇ КОМІРКИ: ВАЛІДАЦІЯ МЕТОДУ ТА ЗАСТОСУВАННЯ

Анотація. Методом диференційної потенціометрії із застосуванням електрохімічної комірки Бауке, розділеної посередині пористою скляною дисковою перегородкою на так звані дві напівкомірки, приготований фталатний буферний розчин як вторинний стандарт для величини рН. Правильність цього методу перевірена за температури 298 К з метою оцінки його придатності. Параметри валідації методу включають точність (відхилення від істинного значення), прецизійність (повторюваність) та оцінку невизначеності вимірювань. Виявлено, що і точність, і прецизійність методу були на належному рівні, що підтверджується дуже низькими величинами стандартних відхилень. Проведено оцінку величини невизначеності вимірювання цього методу. Застосування валідованого аналітичного методу для вимірювання величини рН фталатного буферного розчину згідно міжнародного порівняльного випробування (APMP.QM-K91) показало, що результат був близьким до паспортної (сертифікованої) величини, яка використовується як референтна для порівняння в рамках випробування APMP.QM-K91.

Ключові слова: диференціальна потенціометрична комірка, рН, фталатний буферний розчин, валідація методу, порівняння з міжнародною референтною величиною.